

Whole-Body Dot Engine



The Skyra^{fit} Experience

Editorial Comment

- 2** The Rapid Imaging Renaissance
*Daniel K. Sodickson,
New York University
Langone Medical Center,
New York, NY, USA*



Cover image courtesy of
Andreas J. Bartsch
*(Radiologie Bamberg, Germany;
Departments of Neuroradiology,
Universities of Heidelberg and
Wuerzburg, Germany; Oxford Centre
for Functional MRI of the Brain
(FMRIB), University of Oxford, UK)*

Technology

- 12** Overview of MR Fingerprinting*
*Vikas Gulani, et al.,
Case Western Reserve University,
University Hospitals Case
Medical Center, Cleveland,
OH, USA*
- 22** New Strategies for Protocol
Optimization for Clinical MRI
*Otto Rapalino, et al.,
Massachusetts General Hospital,
Boston, MA, USA*
- 26** Slice Specific Adjustment*
Improves the Image Quality of
Whole-Body Diffusion-Weighted
Examinations at 3T
*Xue Huadan, et al.,
Peking Union Medical College
Hospital, Beijing, China*

Abdominal Imaging

- 31** Whole-Body Dot Engine:
First Clinical Experience with
Automated Chest, Abdomen
and Pelvis Examinations
*Caecilia S. Reiner, et al.,
University Hospital Zurich,
Switzerland*

Pediatric Imaging

- 34** Pictorial Essay:
Pulmonary Imaging for Children¹
*Sonja Kinner, et al.,
University Hospital Essen, Germany*

Business


- 37** The Skyra^{fit} Experience in Basel
*Thomas Egelhof, et al.,
Merian Iselin Spital,
Basel, Switzerland*

Review

- 40** Biograph mMR:
System and Clinical Use Today
*Björn W. Jakoby, et al.,
Siemens Healthcare,
Erlangen, Germany*

Head and Neck Imaging

- 44** Permeability Imaging of Parotid
Tumors with GRASP MR Imaging
*Sohil H. Patel, et al.,
New York University Langone
Medical Center, New York,
NY, USA*

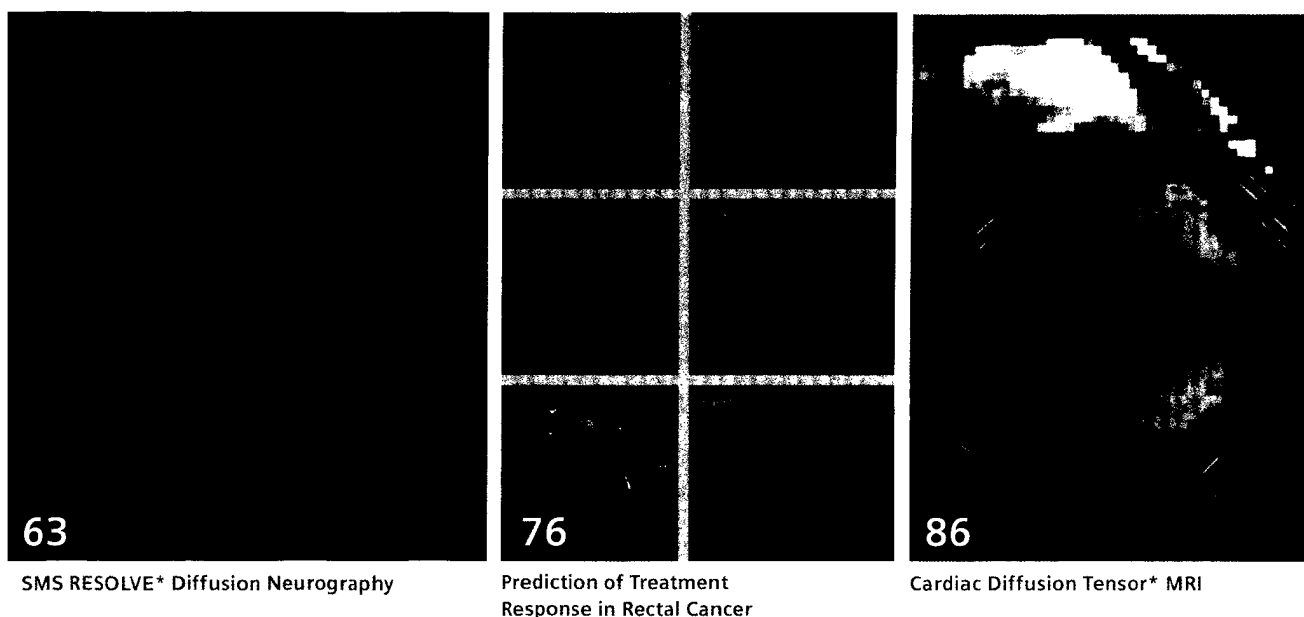

SMS RESOLVE* Diffusion Neurography

Prediction of Treatment Response in Rectal Cancer

Cardiac Diffusion Tensor* MRI

How-I-do-it

46 Further Customization of Dot Engines: AutoCoverage
Bart Schraa,
Siemens Canada Limited,
Oakville, ON, Canada

52 syngo.MR Neuro 3D
Lisa Chuah, et al.,
Siemens Healthcare,
Erlangen, Germany

Musculoskeletal Imaging

63 Case Report:
 High-Resolution SMS RESOLVE*
 Diffusion Neurography
Andreas J. Bartsch,
Radiologie Bamberg, Germany

Women's Health

68 Case Report:
 3D SPACE MR Acquisition in
 Genitourinary Tract Imaging
Priti Apte-Upasani, et al.,
Sun Scan Center, Thane, India

70 Diffusion-Weighted MR
 Mammography. Potential in the
 Clarification of Suspicious Lesions
 Detected by X-Ray Mammography
Sebastian Bickelhaupt, et al.,
German Cancer Research Center
(DKFZ), Heidelberg, Germany

80 Significant Benefit of Optimized
 3D SPACE Sequences in Radiation
 Therapy Treatment
Maja Sohlén, et al.,
Sahlgrenska University Hospital,
Gothenburg, Sweden

82 The Potential Role of Ultrashort
 Echo Time Sequences in
 MRI Guided Radiotherapy
Gary Liney, et al.,
Liverpool Cancer Therapy Centre,
Liverpool Hospital, Sydney,
Australia

Radiation Therapy

76 Multiparametric MRI at 3T
 for Prediction of Treatment
 Response in Rectal Cancer
Trang Pham, et al.,
Liverpool Cancer Therapy Centre,
Liverpool Hospital, Sydney,
Australia

Cardiovascular Imaging

86 Cardiac Diffusion Tensor MRI
Daniel B. Ennis, et al.,
University of California,
Los Angeles, CA, USA

WIP, the product is currently under development and is not for sale in the US and in other countries. Its future availability cannot be ensured. MR scanning has not been established as safe for imaging fetuses and infants less than two years of age. The responsible physician must evaluate the benefits of the MR examination compared to those of other imaging procedures.

The information presented in MAGNETOM Flash is for illustration only and is not intended to be relied upon by the reader for instruction as to the practice of medicine. Any healthcare practitioner reading this information is reminded that they must use their own learning, training and expertise in dealing with their individual patients. This material does not substitute for that duty and is not intended by Siemens Healthcare to be used for any purpose in that regard. The treating physician bears the sole responsibility for the diagnosis and treatment of patients, including drugs and doses prescribed in connection with such use. The Operating Instructions must always be strictly followed when operating the MR system. The source for the technical data is the corresponding data sheets.